


6.

Slide strap under IV tubing and wrap the top strap around the lower leg and the splint.

Lightly tension the straps as they wrap around the back of the splint.




7.

Secure tubing at lower leg with final pass of strap.

Slip strap under loop of tubing at toe.


Wrap the bottom strap over the toes and slip the free end through the hole in the splint near the toes.



8.

Note: Slip one finger beneath each strap to ensure the fabric is not so tight that it impedes circulation or infusion of IV fluids.

Use pre-attached Velcro® hook tabs to secure the ends of the straps.

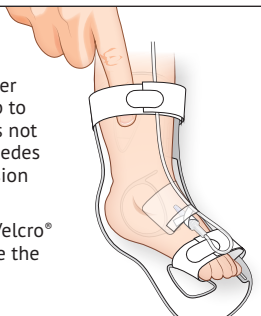

Video Directions: www.ivhouse.com/how

Manufactured for I.V. House, Inc.
2072 Concourse Dr.
St. Louis, MO 63146 USA
IVinfo@ivhouse.com (E-mail)
www.ivhouse.com
800-530-0400 (Toll Free)
314-453-9200 (Phone)
314-453-9576 (Fax)

Patents Pending
All Rights Reserved
Made in USA



Wellkang Enterprise Hub,
NW Business Complex, 1 Beraghmore Rd,
Derry, BT48 8SE, Northern Ireland.



FOOT / INFANT / 6-12 KG

TLC® Foot Splint
Touch/Look/Compare



949S-Foot

1 Small (Infant) Size Foam Padded Foot Splint
with Two Straps and Velcro® Closure

Fits most infants ages 4-12 months,
or weighing 6-12 kg
May fit larger infants, non-ambulatory only

CATALOG ITEM:

REF 949S-Foot



LOT 2022-07-01-949S REV 0722




I.V. HOUSE®
Protection Over and Above®

949S TLC® Foot Splint / Small Foot / Directions

Single Use Only - Fits either foot, laterally or medially.


The TLC Foot Splint can be applied to foot/ankle before or after inserting IV and connecting to extension set or IV tubing.

1.

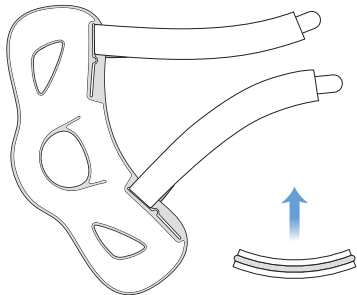


Orient the concave side of the splint facing upward and unroll the straps.

2.

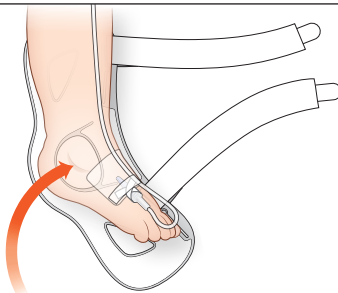


Align the infant's ankle with the splint's middle opening. The heel should roughly coincide with the prominent curve at the outer edge of the splint.

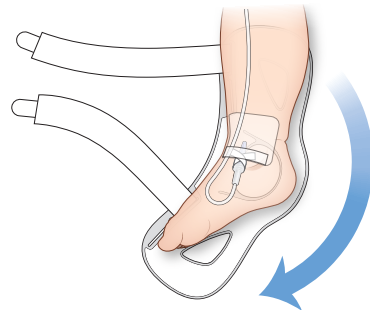


Rotate the splint to position it laterally or medially, on a left or right foot.

3.




Determine which end of the splint will fit to the toe, and which end will fit to the lower leg.

4.

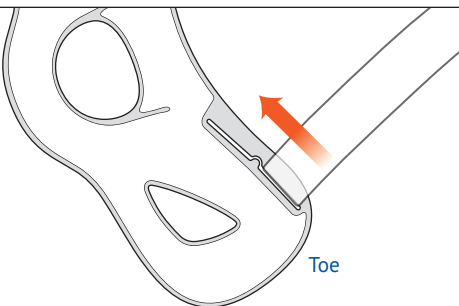

Note that each of the two strap anchor slots has two positions.

5.

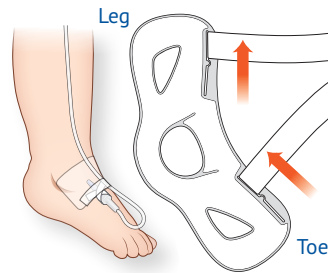

With the splint oriented as it will fit to the infant's foot, slide the strap to the top position in each slot.

Directions continued on back