

949XS TLC® Foot Splint

Touch / Look / Compare

Extra-Small Directions

Single Use Only - Fits either foot, laterally or medially.

The TLC Foot Splint can be applied to foot/ankle before or after inserting IV and connecting to extension set or IV tubing.

1. Orient the concave side of the splint facing upward and unroll the straps.
2. Align the infant's ankle with the splint's middle opening. The heel should roughly coincide with the prominent curve at the outer edge of the splint.
Rotate the splint to position it laterally or medially, on a left or right foot.
3. Slide strap under IV tubing and wrap the top strap around the lower leg and the splint.
Wrap the bottom strap over the toes and slip the free end through the hole in the splint near the toes. Slip strap under loop of tubing at toe.
Lightly tension the straps as they wrap around the back of the splint.
Secure tubing at lower leg with final pass of strap.
4. **Note:** Slip one finger beneath each strap to ensure the fabric is not so tight that it impedes circulation or infusion of IV fluids.
Use pre-attached Velcro® hook tabs to secure the ends of the straps.



Video Directions: www.ivhouse.com/how

Manufactured for I.V. House, Inc.
St. Louis, MO 63146 USA
IVinfo@ivhouse.com (E-mail)
www.ivhouse.com
800-530-0400 (Toll Free)
314-453-9200 (Phone)
314-453-9576 (Fax)

Patents Pending
All Rights Reserved
Made in USA

EC REP Wellkang Ltd (www.ce-marking.eu)
29 Harley St., London W1G 9QR, UK



I.V. HOUSE®
Protection Over and Above®

949XS TLC® Foot Splint

Touch / Look / Compare

CATALOG ITEM:

REF 949XS-Foot

1 Extra-Small (Newborn) Size Foam Padded Foot Splint with Two Straps and Velcro® Closure

LOT 2017-10-01-949XS REV 1017



(01)00686004000255

Fits most infants
ages 0–4 months,
or weighing 2.5–7 kg




949XS TLC® Foot Splint / Extra-Small Foot / Directions

Single Use Only - Fits either foot, laterally or medially.


The TLC Foot Splint can be applied to foot/ankle before or after inserting IV and connecting to extension set or IV tubing.

1.

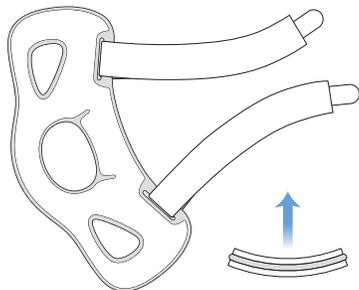


Orient the concave side of the splint facing upward and unroll the straps.

2.

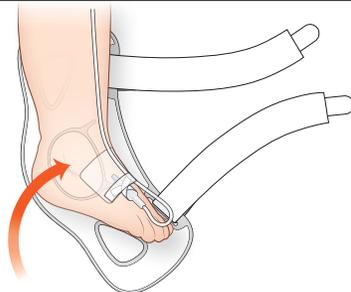

Align the infant's ankle with the splint's middle opening. The heel should roughly coincide with the prominent curve at the outer edge of the splint.

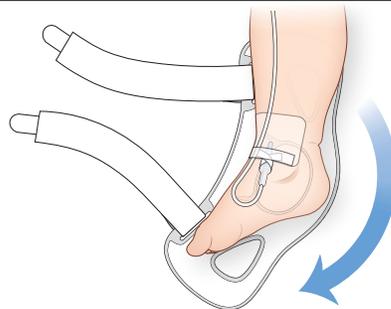


Rotate the splint to position it laterally or medially, on a left or right foot.

3.

Slide strap under IV tubing and wrap the top strap around the lower leg and the splint.

Wrap the bottom strap over the toes and slip the free end through the hole in the splint near the toes.

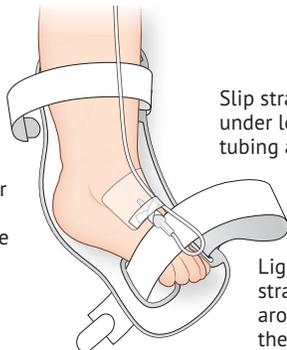

Slip strap under loop of tubing at toe.



Lightly tension the straps as they wrap around the back of the splint.

Secure tubing at lower leg with final pass of strap.

4.

Note: Slip one finger beneath each strap to ensure the fabric is not so tight that it impedes circulation or infusion of IV fluids.

Use pre-attached Velcro® hook tabs to secure the ends of the straps.

